



RptNo. : ETR2642049

第2頁


共2頁

長度部分:

標稱值 (mm)	量測值 (mm)	器差值 (mm)
5.000	5.0003	0.0003
5.005	5.0044	-0.0006
5.020	5.0200	0.0000
5.050	5.0496	-0.0004
5.100	5.1006	0.0006

量測說明:

1. 器差值=量測值 - 標稱值
2. 標稱值係指送量測件所顯示或設定之值
3. 量測值係指工作標準件之輸出值或顯示值
4. 量測能力係以約 95 %信賴水準, $k = 2.00$ 之擴充不確定度表示
5. 擴充不確定度: 0.0040 mm
6. 上述擴充不確定度包含待量測件之不確定度評估結果
7. 量測示意圖:

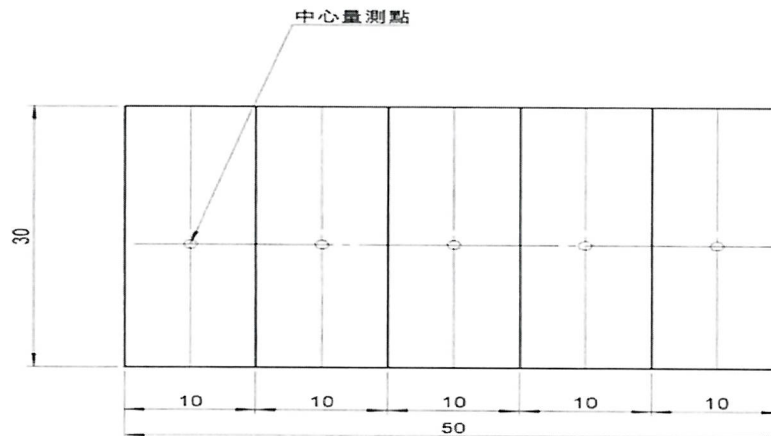

-- THE END --




長度部分:


標稱值 (mm)	量測值 (mm)	器差值 (mm)
5.000	5.0009	0.0009
5.005	5.0053	0.0003
5.020	5.0199	-0.0001
5.050	5.0501	0.0001
5.100	5.1012	0.0012

量測說明:

1. 器差值=量測值 - 標稱值
2. 標稱值係指送量測件所顯示或設定之值
3. 量測值係指工作標準件之輸出值或顯示值
4. 量測能力係以約 95 %信賴水準, $k = 2.00$ 之擴充不確定度表示
5. 擴充不確定度: 0.0040 mm
6. 上述擴充不確定度包含待量測件之不確定度評估結果
7. 量測示意圖:

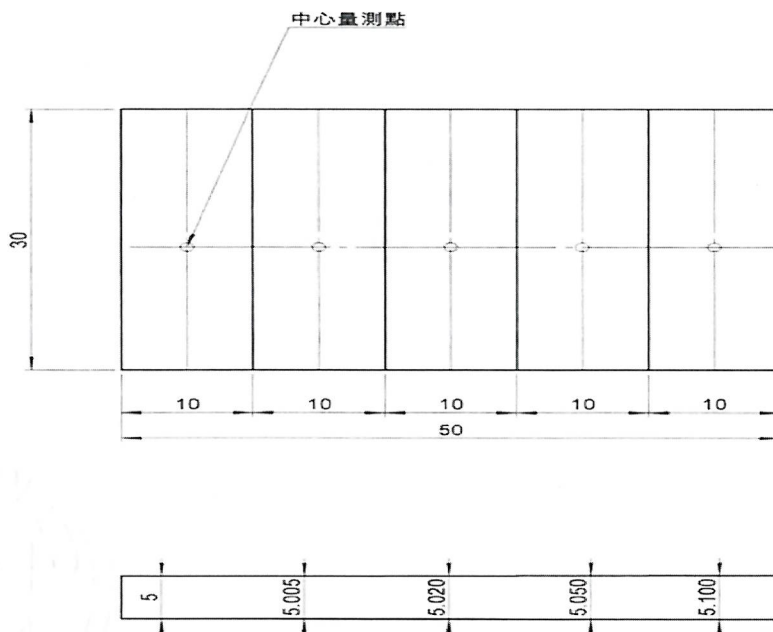

-- THE END --

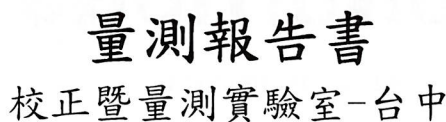

校正暨量測實驗室-台中

報 告 簽 署 人

Member of SGS Group



RptNo. : ETR2642047

第2頁



共2頁

長度部分:

標稱值 (mm)	量測值 (mm)	器差值 (mm)
5.000	5.0001	0.0001
5.005	5.0047	-0.0003
5.020	5.0200	0.0000
5.050	5.0495	-0.0005
5.100	5.1001	0.0001

量測說明:

1. 器差值=量測值 - 標稱值
2. 標稱值係指送量測件所顯示或設定之值
3. 量測值係指工作標準件之輸出值或顯示值
4. 量測能力係以約 95 %信賴水準, $k = 2.00$ 之擴充不確定度表示
5. 擴充不確定度: 0.0040 mm
6. 上述擴充不確定度包含待量測件之不確定度評估結果
7. 量測示意圖:

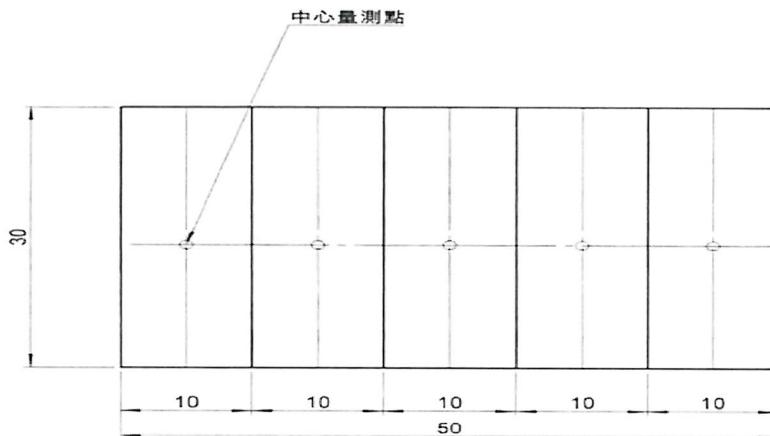

-- THE END --



RptNo. : ETR2642046

第2頁


共2頁

長度部分:

標稱值 (mm)	量測值 (mm)	器差值 (mm)
5.000	5.0010	0.0010
5.005	5.0053	0.0003
5.020	5.0197	-0.0003
5.050	5.0504	0.0004
5.100	5.1008	0.0008

量測說明:

1. 器差值=量測值 - 標稱值
2. 標稱值係指送量測件所顯示或設定之值
3. 量測值係指工作標準件之輸出值或顯示值
4. 量測能力係以約 95 %信賴水準, $k = 2.00$ 之擴充不確定度表示
5. 擴充不確定度: 0.0040 mm
6. 上述擴充不確定度包含待量測件之不確定度評估結果
7. 量測示意圖:

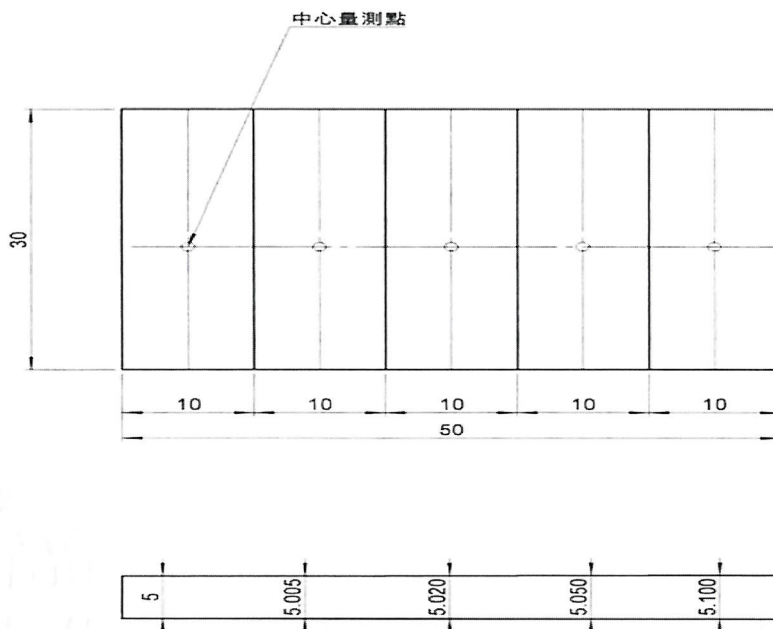

-- THE END --

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <https://www.sgs.com.tw/terms-of-service> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <https://www.sgs.com.tw/terms-of-service>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested in the condition it was received.



RptNo. : ETR2642050

第2頁


共2頁

長度部分:

標稱值 (mm)	量測值 (mm)	器差值 (mm)
5.000	5.0002	0.0002
5.005	5.0053	0.0003
5.020	5.0202	0.0002
5.050	5.0510	0.0010
5.100	5.1001	0.0001

量測說明:

1. 器差值=量測值 - 標稱值
2. 標稱值係指送量測件所顯示或設定之值
3. 量測值係指工作標準件之輸出值或顯示值
4. 量測能力係以約 95 %信賴水準, $k = 2.00$ 之擴充不確定度表示
5. 擴充不確定度: 0.0040 mm
6. 上述擴充不確定度包含待量測件之不確定度評估結果
7. 量測示意圖:

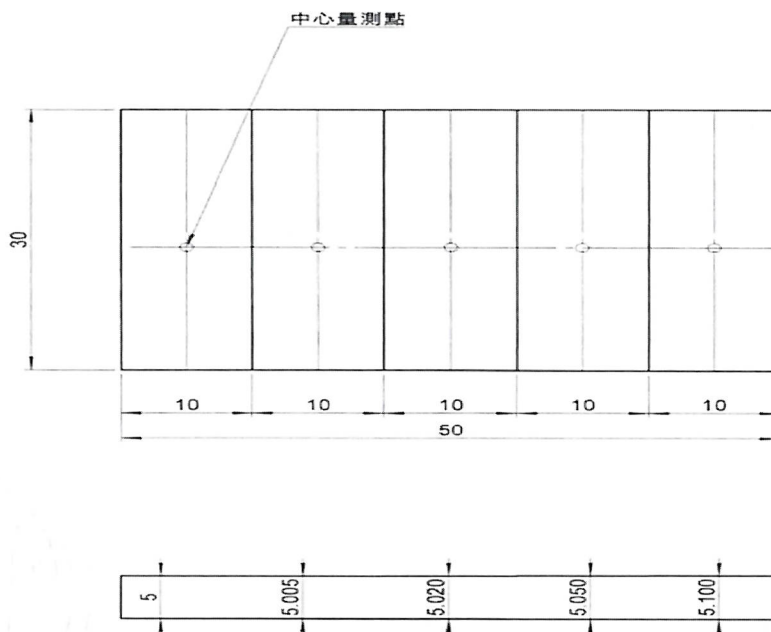

-- THE END --